



THE UNIVERSITY *of* EDINBURGH

Edinburgh Research Explorer

The best practice for preparation of samples from FTA (R) cards for diagnosis of blood borne infections using African trypanosomes as a model system

Citation for published version:

Ahmed, HA, MacLeod, ET, Hide, G, Welburn, SC & Picozzi, K 2011, 'The best practice for preparation of samples from FTA (R) cards for diagnosis of blood borne infections using African trypanosomes as a model system', *Parasites and Vectors*, vol. 4, 68, pp. -. <https://doi.org/10.1186/1756-3305-4-68>

Digital Object Identifier (DOI):

[10.1186/1756-3305-4-68](https://doi.org/10.1186/1756-3305-4-68)

Link:

[Link to publication record in Edinburgh Research Explorer](#)

Document Version:

Publisher's PDF, also known as Version of record

Published In:

Parasites and Vectors

Publisher Rights Statement:

This is an Open Access article distributed under the terms of the Creative Commons Attribution License (<http://creativecommons.org/licenses/by/2.0>), which permits unrestricted use, distribution, and reproduction in any medium, provided the original work is properly cited.

General rights

Copyright for the publications made accessible via the Edinburgh Research Explorer is retained by the author(s) and / or other copyright owners and it is a condition of accessing these publications that users recognise and abide by the legal requirements associated with these rights.

Take down policy

The University of Edinburgh has made every reasonable effort to ensure that Edinburgh Research Explorer content complies with UK legislation. If you believe that the public display of this file breaches copyright please contact openaccess@ed.ac.uk providing details, and we will remove access to the work immediately and investigate your claim.



RESEARCH

Open Access

The best practice for preparation of samples from FTA[®] cards for diagnosis of blood borne infections using African trypanosomes as a model system

Heba A Ahmed^{1,2}, Ewan T MacLeod¹, Geoff Hide³, Susan C Welburn¹ and Kim Picozzi^{1*}

Abstract

Background: Diagnosis of blood borne infectious diseases relies primarily on the detection of the causative agent in the blood sample. Molecular techniques offer sensitive and specific tools for this although considerable difficulties exist when using these approaches in the field environment. In large scale epidemiological studies, FTA[®] cards are becoming increasingly popular for the rapid collection and archiving of a large number of samples. However, there are some difficulties in the downstream processing of these cards which is essential for the accurate diagnosis of infection. Here we describe recommendations for the best practice approach for sample processing from FTA[®] cards for the molecular diagnosis of trypanosomiasis using PCR.

Results: A comparison of five techniques was made. Detection from directly applied whole blood was less sensitive (35.6%) than whole blood which was subsequently eluted from the cards using Chelex[®]100 (56.4%). Better apparent sensitivity was achieved when blood was lysed prior to application on the FTA cards (73.3%) although this was not significant. This did not improve with subsequent elution using Chelex[®]100 (73.3%) and was not significantly different from direct DNA extraction from blood in the field (68.3%).

Conclusions: Based on these results, the degree of effort required for each of these techniques and the difficulty of DNA extraction under field conditions, we recommend that blood is transferred onto FTA cards whole followed by elution in Chelex[®]100 as the best approach.

Background

Blood and buffy coat samples have been routinely collected on ordinary filter paper for analysis and detection of different blood pathogens [1-7]. Although collection of blood samples on filter paper for large scale sampling seems to be more convenient than other sampling procedures, such as *in situ* DNA extraction [2], filter papers are not suitable for long term storage, as they do not protect the sample from spoiling and degradation [8].

Flinders Technology Associates (FTA) technology has improved upon this paper based system. The FTA[®] card has been designed to fix and store nucleic acids directly from tissues, allowing the collection and archiving of nucleic acids [9,10]. The FTA matrix is impregnated

with protein denaturants that cause lysis of cells and any organism on contact. Moreover, these chemicals inhibit detritivores during drying to ensure the safe handling of cards without risk of biohazards [9,11]. FTA technology also includes chelating agents and a free-radical trap designed to deal with atmospheric pollutants, thus protecting the entrapped nucleic acids for at least six years at room temperature [11].

FTA[®] cards have been used for blood storage [12,13], detecting bacterial pathogens [11,14], detection of plant genes [15], specific detection of protozoa in water [16], detection of viral genomes [10,17,18] and in forensic human biology [19]. The use of FTA[®] cards has been extended to include DNA detection from pathogenic protozoa and pathogenic organisms isolated from food and clinical specimens using PCR [20].

The feasibility of FTA[®] cards for the shipment, storage and detection of RNA rabies virus has recently been evaluated by Picard-Meyer *et al.* [10]. The authors

* Correspondence: kim.picozzi@ed.ac.uk

¹Centre for Infectious Diseases, Division of Pathway Medicine, School of Biomedical Sciences, College of Medicine and Veterinary Medicine, University of Edinburgh, 49 Little France Crescent, Edinburgh, EH16 4SB, UK
Full list of author information is available at the end of the article

concluded that the chemicals impregnated in the filter paper have made the samples no longer infectious; subsequently the samples do not induce any biohazards especially during shipment. Moreover, the use of FTA[®] cards facilitates the large scale field sampling of viruses infecting plants and yields DNA with sufficient stability, quantity and quality for further screening over time of storage at room temperature was reported [18]. The authors successfully extracted viral DNA from FTA[®] cards stored at room temperature for nine months.

In trypanosome diagnosis, FTA[®] cards have been used for the storage of many materials including blood, buffy coat and extracted DNA [21-26]. The use of FTA[®] cards for storage of midgut material originating from tsetse flies has been documented by Adams *et al.* [27,28]. They noticed lower trypanosome detection using PCR than was expected and suggested several reasons for this, including the sub-optimum binding of trypanosome DNA to the FTA[®] cards and the uneven binding of the trypanosome DNA throughout the card due to competition with midgut material. The uneven distribution was reported to be the main contributing factor to this decreased sensitivity and that this was compounded when examining infections with low parasite densities [29]. Although FTA[®] cards are a reliable medium for storage and transport of blood samples for PCR-based assays, long-term storage (>9 months) has been shown to prevent the complete removal of blood proteins from discs by washing [23].

The present study was aimed at investigating the best approach for the preparation of blood samples applied on FTA[®] cards for the molecular diagnosis of trypanosomes. This aim was achieved by comparing three sample preparations: whole blood applied directly onto FTA[®] cards, lysed blood on FTA[®] cards and DNA extracted directly in the field using commercial kits. Lysed blood, where the genetic material within the sample was released from the cellular membranes prior to FTA[®] card application, was examined as a possible solution to overcome the localization of DNA across the surface of the membrane. Additionally, the use of Chelex[®] 100 resin (previously described by Becker *et al.* [23] for elution of trypanosome material from FTA cards) was investigated as a possible approach to elute DNA from preprepared FTA[®] cards. These five protocols were compared to establish the most successful method of detection of trypanosome infections from FTA[®] cards.

Results

Three different sample preparations were collected from 300 animals. These preparations included, whole blood applied on FTA[®] cards, lysed blood on FTA[®] cards and direct purification of DNA from blood in the field. Ten discs from each FTA[®] card applied blood sample were

examined individually using TBR-PCR for the detection of *T. brucei* s.l. The sensitivity of the tests were calculated compared to the gold standard which was defined as the total number of PCR positive results from amplification of trypanosome DNA from samples applied to FTA[®] cards and/or from directly extracted trypanosome genomic DNA. Figure 1 shows that there is an increase in cumulative sensitivity as the number of individually examined discs was increased. The same phenomenon was observed from both whole and lysed blood samples.

For whole blood the sensitivity of PCR screening of up to five discs remained constant at 5.9%, compared to the gold standard, which increased to 35.6% when 10 separate discs were examined (Table 1). The sensitivity of detection of lysed blood samples increased from 12.9% by examining 1-2 discs to 73.3% by screening 10 discs when compared to the gold standard. Therefore the release of the genomic material from both the host and any infectious agent into a homogenous solution prior to application of the sample onto FTA[®] cards significantly improved the detection ($p < 0.0001$).

However, although the lysis approach improved sensitivity, it is costly and time consuming to use due to the numerous individual PCR reactions per sample. In order to reduce these overheads, genomic material was eluted from 10 washed discs by collectively heating the preparation at 90°C in the presence of 60 µl of 5% (w/v) aqueous suspension of Chelex 100[®] resin. Five microlitres of eluted DNA extract from each sample was examined by PCR in single reaction and the sensitivity of the different preparations were compared to the gold standard defined above for further evaluation of the lysis and elution protocols (Table 1).

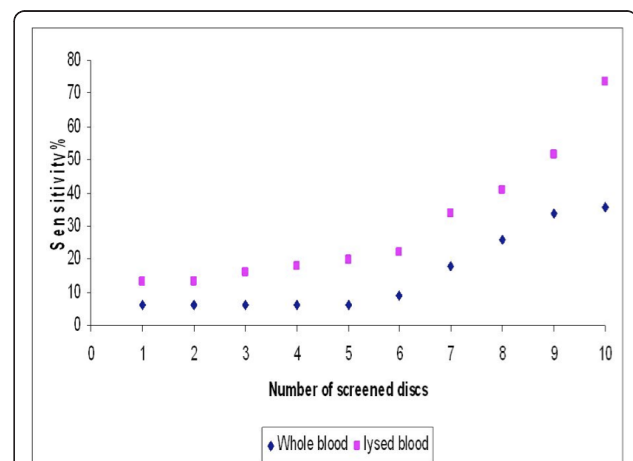


Figure 1 Cumulative number of examined FTA discs containing whole and lysed blood in relation to the sensitivity of detecting the trypanosome DNA by PCR.

Table 1 Sensitivity of the used sample preparations compared to the gold standard for identifying *T. brucei* s.l. by PCR (n = 300)

Material	True positive	False positive	True negative	False negative	% NPV (95%CI)	% Sensitivity (95%CI)	Kappa value
Whole blood on FTA® cards (10 separate discs)	36	0	199	65	75.4% (70.2-80.6)	35.6% (26.3-45)	0.4
Whole blood on FTA® cards (elution)	57	0	199	44	81.9% (77.1-86.7)	56.4% (46.8-66.1)	0.6
DNA extract	69	0	199	32	86.1% (81.7-90.6)	68.3% (59.2-77.4)	0.7
Lysed blood on FTA® cards (elution)	74	0	199	27	88.1% (83.8-92.3)	73.3% (64.6-81.9)	0.8
Lysed blood on FTA® cards (10 separate discs)	74	0	199	27	88.1% (83.8-92.3)	73.3% (64.6-81.9)	0.8

The results show that the sensitivity of a single PCR reaction using 5 µl of DNA eluted with Chelex® 100 solution from 10 discs containing whole blood significantly increased the sensitivity from 35.6% to 56.4% (Table 1) compared to non eluted whole blood taken from 10 separate discs ($\chi_1^2 = 7.3$, $p = 0.007$). A comparison of the sensitivity of detection of *T. brucei* s.l. DNA from lysed blood with Chelex® 100 eluted samples from the lysed blood showed no difference (Table 1). A comparison of the sensitivity of using Chelex® 100 eluates from whole and lysed blood showed an increase from 56.4% to 73.3% but this was not significant ($\chi_1^2 = 1.7$, $p = 0.2$). When comparing the PCR detection sensitivity of Chelex® 100 eluates of whole blood (56.4%) and lysed blood (73.3%) with DNA extracted directly in the field (68.3%) there was no significant difference. Therefore, these two PCR detection protocols based on Chelex® 100 elution are comparable in sensitivity to DNA prepared directly under field conditions at the point of collection.

Table 1 shows the Kappa values for the degree of agreement between the amplification of *T. brucei* s.l. using different preparation and processing methods compared to the gold standard. There was fair agreement between the detection of the DNA in whole blood samples using separate 10 discs for the PCR and the gold standard. Moderate agreement was seen when amplifying the parasite genomic material from eluates of whole blood discs, good agreement was observed in the amplification of DNA extracted in the field and very good agreement was found for both lysed blood samples. However, the lack of significant difference in sensitivity between the latter four processes suggests that each show equally good agreement with the gold standard.

Discussion

FTA cards are considered reliable medium for the storage and transport of blood samples for molecular diagnosis of blood borne infectious diseases. The most important obstacle of processing the samples from the card matrix is the localized trapping of the genomic

material after application of the sample. Moreover, long-term storage of the sample might hinder the release of the entrapped DNA from the card matrix for molecular diagnosis. This study aimed to investigate the application and processing of blood samples on the FTA matrix to improve the detection of trypanosomes by PCR.

The sensitivity of detecting positive discs containing whole blood was constant at 5.9% using one to five discs, after which the sensitivity increased to reach a maximum of 35.6% when all 10 discs were included (Figure 1). This was due to increasing the chance of obtaining parasite DNA in the examined disc as demonstrated previously by Cox *et al.* [29]. However, using discs containing lysed blood samples, the sensitivity of detecting positive discs using PCR increased to 73.3% using 10 discs. Comparing the sensitivity of examining one disc containing whole blood and lysed blood (5.9% and 12.9%, respectively), it was noticed that the lysis step doubled the sensitivity of the screening protocol; this was also the case when comparing the sensitivity of examining 10 discs from the two preparations using separate PCR reactions (35.6% and 73.3%, respectively).

The improvement in detection trypanosome target sequence was clear using the lysed blood samples; however, it required the screening of at least 10 discs to achieve a sufficient sensitivity when compared to the gold standard. The use of increased numbers of discs improved detection due to the increased chance of selecting a region of the card where parasitic DNA was stored. Although using a single disc screening protocol may be valid where infection intensities are generally very high, it may completely underestimate prevalence if the infection intensities are generally very low in the population [29]. Therefore, in order to decrease the probability of false negative results from using a single disc, examination of more discs would give more accurate estimation of the disease prevalence.

Despite the higher sensitivity of examining more discs, the use of 10 discs from whole blood or lysed blood samples with a separate PCR reaction on each disc was considered time consuming and expensive. Moreover,

the use of 10 discs for detecting each trypanosome species would quickly use all the archived material on the card matrix. This was overcome by elution of DNA from FTA[®] cards containing either whole blood or lysed blood using 5% Chelex[®]100 resin aqueous suspension [23]. In both cases, this approach gave a sensitivity that was no different to the 10 disc approach using the TBR-PCR. The sensitivity of using lysed blood eluate in detecting trypanosome DNA was not significantly different than the PCR detection from DNA directly extracted in the field suggesting that these methods are as good and also more convenient alternatives.

Relating parasite density to PCR positivity on FTA cards can be problematic, however, Cox *et al.* [29] have recently suggested that the level of parasitaemia is related to the number of punches that are positive. Hence if 1/8 punches are positive the infection rate is 0.1 trypanosome per ml, 6/8 punches positive represents one trypanosome per ml and finally a 100% detection rate where there are greater than 10 parasites per ml. In the current work, however, sensitivity was increased by either elution of DNA or pre lysis of material before application to FTA card. This would suggest that parasite densities could be higher than those suggested by PCR from FTA cards. Although this would not affect the positivity status when parasitaemia was high it could have an affect when measuring density in low parasitaemias (particularly if trypanosomes clumped in particular areas of the card). Becker *et al.* [23] have published a quantitative real time method for the enumeration of trypanosomes from FTA card and this could provide an approach for measuring trypanosome populations from FTA samples. However, given the fact that trypanosome populations do fluctuate (due to antigenic variation) assessing if the animal is positive is more important in prevalence studies than the number of trypanosomes present in the animal.

Research has focused on the development of alternative extraction protocols that overcome the drawbacks of the conventional methods, but at the same time producing efficient DNA yield in both the quantity and quality to be easily amplified using PCR [30]. DNA elution from blood applied on FTA[®] cards or filter papers using 5% aqueous Chelex[®]100 solutions appear to be more convenient and cheaper than DNA extraction using extraction kits [23]. Other studies have shown that the benefits from using Chelex[®]100 to extract DNA from blood result in a six-fold increase in extraction efficiency [31] although in our study it only doubled the sensitivity. However, these approaches are better than conventional methods of DNA extraction that require large volumes of blood and the use of health hazard organic solvents [32]. A demonstration of the universal usefulness of Chelex[®]100 is that it has been used to

elute the genomic DNA from a range of other parasites immobilized on filter paper including *Theileria parva* [30,33] and *Plasmodium falciparum* [34]. In the case of trypanosomes it has been used to elute from filter paper [1,6,35-38], buffy coat [2,38,39] and CSF [40]. Our study demonstrates the important application of it for use with FTA cards.

From the previous studies, it is clear that the use of Chelex[®]100 is effective in stabilizing the extraction of highly pure DNA from blood samples that are notorious for the carryover of PCR inhibitors [30]. The presence of Chelex overcomes the problems associated with inhibitory effects of the blood components such as heme, lactoferrin, IgG and non-target DNA [29,35]. Moreover, Chelex[®]100 protects DNA from the effects of high temperature that can cause degradation of DNA by chelating metal ions which might act as catalysts in the breakdown of DNA at high temperature in low ionic strength solutions [41].

DNA extraction from different samples including blood, CSF, tissues and cultures is an important step for conducting PCR for the diagnosis and research purposes. Extraction of DNA using different kits has been proven to recover high molecular weight DNA but this process is time consuming and expensive. Moreover, these methods require several steps and may include the transfer of DNA extracts to additional containers and columns increasing the chance for cross-transfer of samples or the introduction of contaminants [42]. ChargeSwitch[®] gDNA kit used in this study to extract DNA from blood did not require the use of any electrical equipment because it depends on the use of magnetic beads, however, it was time consuming and expensive. For extracting DNA from one sample using ChargeSwitch[®] gDNA kit, the cost was £4.20 compared to £2.70 and £3.20 (2010 prices) using whole blood and lysed blood on FTA[®] cards, respectively.

In conclusion, successful molecular diagnosis requires the availability of genomic material of an appropriate quality and concentration to be present within the sample under examination. The insignificant difference between using DNA eluted (by Chelex[®]100) from whole blood, lysed blood discs and DNA extracted using kits, suggests that the use of any of these aforementioned preparations are suitable for obtaining trypanosome genomic materials for molecular analysis. The choice will therefore be based on economic and time factors. Direct DNA extraction in the field using kits can be excluded due to the expensive kits and time taken for extracting DNA.

Conclusions

The current work recommends that whole blood samples are collected using FTA[®] card technology with

DNA being eluted using Chelex[®]100 once the investigator has returned to the laboratory. These steps should increase the sensitivity of the molecular diagnosis of trypanosome infections as it overcomes any problems associated with uneven distribution of parasite DNA on the card matrix.

Methods

Sample collection

In this study three sample preparations were collected under field conditions from 300 cattle from Apac and Lira districts, from Uganda during baseline sampling of the Stamp out Sleeping Sickness campaign in 2006 [43]. These preparations included whole and lysed blood applied on FTA[®] cards and DNA extracted using ChargeSwitch[®] gDNA kits. The lysed blood was obtained by 1:1 dilution of the blood sample using sterile water, after allowing time for lysis to take place; the sample was then applied to the FTA matrix.

Preparation of samples

For samples applied on FTA[®] cards, 0.2 mm discs were cut from the card for PCR analysis. The number of discs to be examined were cut and placed together into a micro-centrifuge tube for washing. To avoid cross contamination between samples, an equivalent number of discs were taken from a blank filter paper after each sample. The discs were washed twice, for 15 minutes each, in 200 µl (for each disc) of Whatman FTA purification reagent. The discs were then washed twice for 15 minutes in 200 µl (for each disc) 1 mM TE buffer (10 mM Tris-HCL pH 8.0; 1 mM EDTA pH 8.0), were then transferred to PCR tubes and left to dry at room temperature for at least 90 minutes [21]. Ten discs from both whole blood and lysed blood FTA[®] card preparations were examined by PCR (each disc examined with a separate PCR reaction).

The DNA from a further 10 prepared discs from each FTA[®] card sample was eluted collectively by heating the discs for 30 minutes at 90°C in 60 µl of 5% (w/v) aqueous suspension of Chelex 100[®] resin (sodium form, 50-100 dry mesh, Sigma) [23]. For PCR, 5 µl of the eluate was added to 20 µl of the PCR master mix.

DNA extraction directly from field sampling was carried out according to the manufacturer using the ChargeSwitch[®] gDNA kit. The principle of this extraction method is the use of magnetic beads. At low pH, the magnetic beads have a positive charge that binds the negatively charged nucleic acid backbone of DNA. Proteins and other contaminants do not bind and are removed by washing. For the elution of the bound DNA, the charge of the magnetic beads was neutralised by raising the pH to 8.5 using a low salt elution buffer. The purified DNA was released into the elution buffer;

the yield from 50 µl of blood was up to 2 µg. For PCR, 1 µl from the extract was used as the template.

PCR

TBR-PCR was used in the current study for the detection of *T. brucei* s.l. The reaction is species specific, amplifying a 173 bp product from a repetitive satellite sequence of 177 bp size [44]. The copy number of the satellite sequence was reported to be 10,000 copies/genome [45] ensuring high sensitivity. The primer sequences used were TBR1-5'-CGA ATG AAT ATT AAA CAA TGC GCA GT-3' and TBR2-5'-AGA ACC ATT TAT TAG CTT TGT TGC-3' [44].

The reaction volume used was 25 µl and contained NH₄ Buffer (Bioline, London, UK) which comprises 16.0 mM (NH₄)₂SO₄, 67 mM Tris-HCl (pH 8.8 at 25°C) and 0.01% Tween 20. Moreover, 0.4 µM of each primer, 1.5 mM Mg²⁺, 200 µM of each of the four-deoxynucleoside triphosphates (dNTP) and one Unit of BIOTAQ RED DNA Polymerase (Bioline) were added. One positive control (genomic DNA) and one negative control were run with each PCR. The reaction conditions used were as follows: 1 cycle of 95°C for seven minutes followed by 30 cycles of 94°C for one minute, 55 °C for one minute and 72 °C for 30 seconds. The reaction was carried out in a DNA Engine DYADTM Peltier Thermal Cycler. Amplified products were visualized on a 1% (w/v) agarose gel electrophoresis.

Data analysis

The difference in trypanosome detection between the different sample preparations was analysed using the Chi-squared test (the degrees of freedom were noted as a subscript to the χ^2 -statistic) and was computed using Minitab version 15 (Minitab, Inc.). Differences were considered to be significant at $p < 0.05$. For values containing expected frequencies of less than five, Fisher's exact test was used instead of the Chi-squared test. The Kappa value was used to determine the level of agreement between the diagnostic test and the gold standard. The Kappa value lies between 0 and 1, where the following definitions apply: 0.8-1, very good agreement between tests; 0.6-0.8, good agreement; 0.4-0.6, moderate agreement; 0.2-0.4, fair agreement; 0-0.2, poor agreement; 0, the association is no better than expected from chance alone, a negative Kappa value indicates that the two tests agree less than would be expected by chance [46,47].

Acknowledgements

HAA would like to show a sincere gratitude to the Egyptian government represented in the public administration missions and the culture bureau in the United Kingdom for the financial and moral support that had a real impact on my research. SCW and ETM are members of COST Action

BM0802, Life or Death of Protozoan Parasites. SCW and KP acknowledge support of DFID Research Into Use Programme, ICONZ, (Integrated Control of Neglected Zoonoses) an EU FP7 project and the BBSRC through CIDLID. Thanks to Richard Selby and the SOS team for collecting the Uganda samples during the follow up. We are also grateful to Dr. Darren Shaw for his statistical advice.

Author details

¹Centre for Infectious Diseases, Division of Pathway Medicine, School of Biomedical Sciences, College of Medicine and Veterinary Medicine, University of Edinburgh, 49 Little France Crescent, Edinburgh, EH16 4SB, UK. ²Faculty of Veterinary Medicine, Zagazig University, 44611, Egypt. ³Centre for Parasitology and Disease, School of Environment and Life Sciences, University of Salford, Salford, M5 4WT, UK.

Authors' contributions

HAA carried out the study, the molecular approaches and participated in preparing the manuscript. ETM participated in preparing and editing the manuscript. GH participated in editing the manuscript. SCW designed the study supervised the molecular approaches and participated in preparing and editing the manuscript. KP designed the study supervised the molecular approaches and participated in preparing and editing the manuscript. All authors read and approved the final manuscript.

Competing interests

The authors declare that they have no competing interests.

Received: 23 March 2011 Accepted: 7 May 2011 Published: 7 May 2011

References

1. Boid R, Jones TW, Munro A: A simple procedure for the extraction of trypanosome DNA and host protein from dried blood meal residues of haematophagous diptera. *Vet Parasitol* 1999, **85**:313-317.
2. de Almeida PP, Ndao M, Van Meirvenne N, Geerts S: Diagnostic evaluation of PCR on dried blood samples from goats experimentally infected with *Trypanosoma brucei*. *Act Trop* 1998, **70**:269-276.
3. Delespaux V, Ayrat F, Geysen D, Geerts S: PCR-RFLP using Ssu-rDNA amplification: applicability for the diagnosis of mixed infections with different trypanosome species in cattle. *Vet Parasitol* 2003, **117**:185-193.
4. Gonzales JL, Jones TW, Picozzi K, Cuellar HR: Evaluation of a polymerase chain reaction assay for the diagnosis of bovine trypanosomiasis and epidemiological surveillance in Bolivia. *Kinetoplastid Biol Dis* 2003, **2**(8):1-14.
5. Goossens B, Mbwambo H, Msangi A, Geysen D, Vreysen M: Trypanosomiasis prevalence in cattle on Mafia Island (Tanzania). *Vet Parasitol* 2006, **1**-10.
6. Katakura K, Lubinga C, Chitambo H, Tada Y: Detection of *Trypanosoma congolense* and *T. brucei* subspecies in cattle in Zambia by polymerase chain reaction from blood collected on a filter paper. *Parasitol Res* 1997, **83**:241-245.
7. Mahama CI, Desquesnes M, Dia ML, Losson B, De Deken R, Geerts S: A cross-sectional epidemiological survey of bovine trypanosomiasis and its vectors in the Savelugu and West Mamprusi districts of northern Ghana. *Vet Parasitol* 2004, **122**:1-13.
8. Smith LM, Burgoyne LA: Collecting, archiving and processing DNA from wildlife samples using FTA® databasing paper. *BMC Ecol* 2004, **4**(4):1-11.
9. Belgrader P, Del Rio SA, Turner KA, Marino MA, Weaver KR, Williams PE: Automated DNA purification and amplification from blood stained cards using a robotic workstation. *Biotechniques* 1995, **19**(3):426-432.
10. Picard-Meyer E, Barrat J, Cliquet F: Use of filter paper (FTA®) technology for sampling, recovery and molecular characterisation of rabies viruses. *J Virol Meth* 2007, **140**:174-182.
11. Rogers C, Burgoyne LA: Bacterial typing: storing and processing of stabilized reference bacteria for polymerase chain reaction without preparing DNA-an example of an automatable procedure. *Anall Biochem* 1997, **247**:223-227.
12. Devost NC, Choy FYM: Mutation analysis of gaucher disease using dot-blood samples on FTA® filter paper. *Am J Med Genet* 2000, **94**:417-420.
13. Gutierrez-corchero F, Arruga MV, Sanz L, Garcia C, Hernandez AM, Campos F: Using FTA® cards to store avian blood samples for genetic studies. Their application in sex determination. *Mol Ecol Notes* 2002, **2**:75-77.
14. Lampel KA, Orlandi PA, Kornegay L: Improved template preparation for PCR-based assays for detection of food-borne bacterial pathogens. *Appl Environ Microbiol* 2000, **66**(10):4539-4542.
15. Lin JJ, Fleming R, Matthews BF, Saunders JA: Detection of plant genes using a rapid, nonorganic DNA purification method. *Biotechniques* 2000, **28**(2):346-350.
16. Hide G, Hughes JM, McNuff R: A rapid and simple method of detection of *Blepharisma japonicum* using PCR and immobilisation on FTA paper. *BMC Ecol* 2003, **3**:7.
17. Ndunguru J, Taylor N, Yadav J, Aly H, Legg J, Aveling T, Thompson G, Fauquet C: Application of FTA technology for sampling, recovery and molecular characterization of viral pathogens and virus-derived transgenes from plant tissues. *Virology* 2005, **2**:45.
18. Owor BE, Shepherd DN, Taylor NJ, Edema R, Monjane AL, Thomson JA, Martin DP, Varsani A: Successful application of FTA® Classic Card technology and use of bacteriophage [phi]29 DNA polymerase for large-scale field sampling and cloning of complete maize streak virus genomes. *J Virol Methods* 2007, **140**:100-105.
19. Hedman J, Albinsson L, Ansell C, Tapper H, Hansson O, Holgersson S, Ansell R: A fast analysis system for forensic DNA reference samples. *J Forensic Sci Int Genet* 2008, **2**:184-189.
20. Orlandi PA, Lampel KA: Extraction-free, filter-based template preparation for rapid and sensitive PCR detection of pathogenic parasitic protozoa. *J Clin Microbiol* 2000, **38**(6):2271-2277.
21. Picozzi K, Tilley A, Fevre EM, Coleman PG, Magona JW, Oditt M, Eisler MC, Welburn SC: The diagnosis of trypanosome infections: applications of novel technology for reducing disease risk. *African J Biotech* 2002, **1**(2):39-45.
22. Picozzi K, Fevre EM, Odiit M, Carrington M, Eisler MC, Maudlin I, Welburn SC: Sleeping sickness in Uganda: a thin line between two fatal diseases. *BMJ* 2005, **331**:1238-1241.
23. Becker S, Franco JR, Simarro PP, Stich A, Abel PM, Steverding D: Real-time PCR for detection of *Trypanosoma brucei* in human blood samples. *Diagn Microbiol Infect Dis* 2004, **50**(3):193-199.
24. Cox A, Tilley A, McOdimba F, Fyfe J, Eisler MC, Hide G, Welburn SC: A PCR based assay for detection and differentiation of African trypanosome species in blood. *Exp Parasitol* 2005, **111**:24-29.
25. Kaare MT, Picozzi K, Mlengeya T, Fevre EM, Mellau LS, Mtambo MM, Cleaveland S, Welburn SC: Sleeping sickness- A re-emerging disease in the Serengeti? *Travel Med Infect Dis* 2007, **5**:117-124.
26. Salim B, Bakheit MA, Kamau J, Nakamura I, Sugimoto C: Molecular epidemiology of camel trypanosomiasis based on ITS1 rDNA and RoTat 1.2 VSG gene in the Sudan. *Parasit Vectors* 2011, **4**:31.
27. Adams ER, Malele II, Msangi AR, Gibson WC: Trypanosome identification in wild tsetse populations in Tanzania using generic primers to amplify the ribosomal RNA ITS-1 region. *Act Trop* 2006, **100**:103-109.
28. Adams ER, Hamilton PB, Malele II, Gibson WC: The identification, diversity and prevalence of trypanosomes in field caught tsetse in Tanzania using ITS-1 primers and fluorescent fragment length barcoding. *Infect Genet Evol* 2008, **8**:439-444.
29. Cox AP, Tosas O, Tilley A, Picozzi K, Coleman P, Hide G, Welburn SC: Constraints to estimating the prevalence of trypanosome infections in East African zebu cattle. *Parasit Vectors* 2010, **3**:82.
30. Polski JM, Kimzey S, Percival RW, Grosso LE: Rapid and effective processing of blood specimens for diagnostic PCR using filter paper and Chelex-100. *Mol Pathol* 1998, **51**:215-217.
31. Jung JM, Comey CT, Baer DB, Budowle B: Extraction strategy for obtaining DNA from bloodstains for PCR amplification and typing of the HLA-DQ alpha gene. *Int J Legal Med* 1991, **104**:145-148.
32. Loparev VN, Cartas MA, Monken CE, Velpandi A, Srinivasan A: An efficient and simple method of DNA extraction from whole blood and cell lines to identify infectious agents. *J Virol Methods* 1991, **34**:105-112.
33. Geysen D, Bishop R, Skilton R, Dolan TT, Morzaria S: Molecular epidemiology of *Theileria parva* in the field. *Trop Med Int Health* 1999, **4**(9):A21-A27.
34. Wooden J, Kyes S, Sibley CH: PCR and strain identification in *Plasmodium falciparum*. *Parasitol Today* 1993, **9**(8):303-305.
35. de Almeida PJLP, Ndao M, Van Meirvenne N, Geerts S: Diagnostic evaluation of PCR in goats experimentally infected with *Trypanosoma vivax*. *Act Trop* 1997, **66**:45-50.

36. de Almeida PJL, Ndao M, Goossens B, Osaer S: **PCR primer evaluation for the detection of trypanosome DNA in naturally infected goats.** *Vet Parasitol* 1998, **80**:111-116.
37. Jamonneau V, Ravel S, Koffi M, Kaba D, Zeze DG, Ndri L, Sane B, Coulibaly B, Cuny G, Solano P: **Mixed infections of trypanosomes in tsetse and pigs and their epidemiological significance in a sleeping sickness focus of Cote d'Ivoire.** *Parasitol* 2004, **129**:693-702.
38. Solano P, Jamonneau V, N'Guessan P, N'Dri L, Dje NN, Miezian TW, Lejon V, Buscher P, Garcia A: **Comparison of different DNA preparation protocols for PCR diagnosis of human African trypanosomiasis in Cote d'Ivoire.** *Act Trop* 2002, **82**:349-356.
39. Solano P, Michel JF, Lefrancois T, de La Rocque S, Sidibe I, Zoungrana A, Cuisance D: **Polymerase chain reaction as a diagnosis tool for detecting trypanosomes in naturally infected cattle in Burkina Faso.** *Vet Parasitol* 1999, **86**:95-103.
40. Truc P, Jamonneau V, Cuny G, Frezil JL: **Use of polymerase chain reaction in human African trypanosomiasis stage determination and follow-up.** *Bull WHO* 1999, **77**:745-748.
41. Singer-Sam J, Tanguay RL, Riggs AD: **Use of Chelex to improve the PCR signal from a small number of cells.** *Amplifications: A forum for PCR users* 1989, **11**.
42. Walsh PS, Metzger DA, Higuchi R: **Chelex 100 as a medium for simple extraction of DNA for PCR-based typing from forensic material.** *Biotechniques* 1991, **10**:506-513.
43. Ahmed HA: **African trypanosomes; a model for the improvement of molecular diagnosis of blood borne parasites.** Edinburgh University; 2009, PhD thesis.
44. Moser DR, Cook GA, Ochs DE, Bailey CP, McKane MR, Donelson JE: **Detection of *Trypanosoma congolense* and *Trypanosoma brucei* subspecies by DNA amplification using the polymerase chain reaction.** *Parasitol* 1989, **99**:57-66.
45. Sloof P, Bos JL, Konings AF, Menke HH, Borst P, Gutteridge WE, Leon W: **Characterization of satellite DNA in *Trypanosoma brucei* and *Trypanosoma cruzi*.** *J Mol Biol* 1983, **167**:1-21.
46. Altman DG: **Practical statistics for medical research.** London, England; 1991, Chapman and Hall.
47. Cohen JE: **A coefficient of agreement for nominal scales.** *Edu Psychol Meas* 1960, **20**:37-46.

doi:10.1186/1756-3305-4-68

Cite this article as: Ahmed *et al.*: The best practice for preparation of samples from FTA[®] cards for diagnosis of blood borne infections using African trypanosomes as a model system. *Parasites & Vectors* 2011 **4**:68.

**Submit your next manuscript to BioMed Central
and take full advantage of:**

- Convenient online submission
- Thorough peer review
- No space constraints or color figure charges
- Immediate publication on acceptance
- Inclusion in PubMed, CAS, Scopus and Google Scholar
- Research which is freely available for redistribution

Submit your manuscript at
www.biomedcentral.com/submit

